



NOBLE

Split-Specimen Cup®

1 Collect Specimen

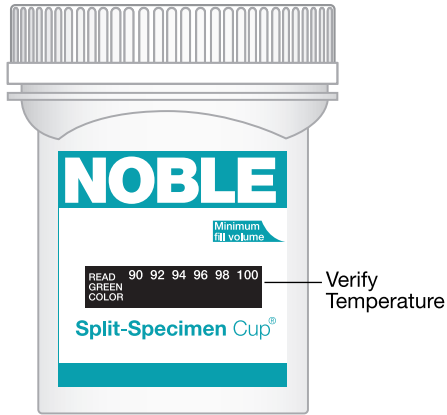


2 Insert Key

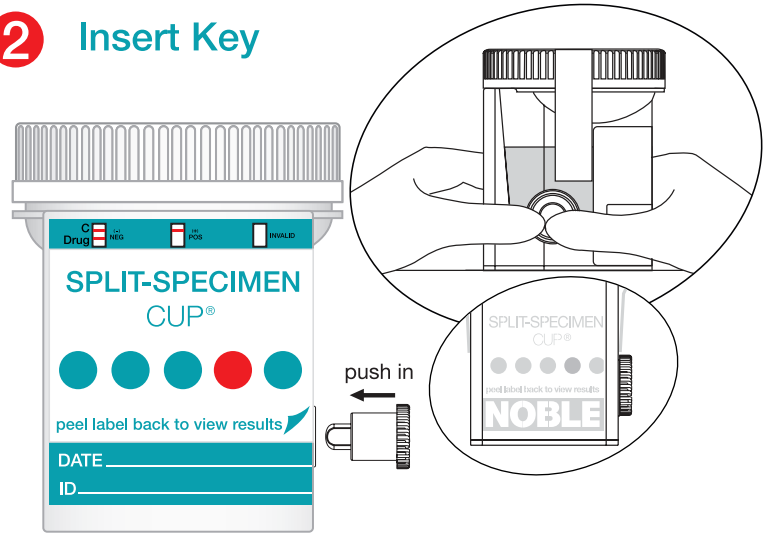

3 Peel Back Label




4 Read the Results

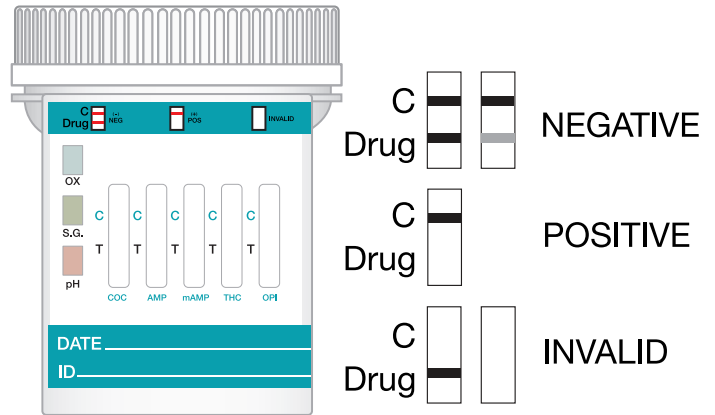

All positive results are presumptive and should be confirmed by an alternate method. (e.g. GC/MS)



Read results at (5) minutes.
Results stable up to (60) minutes.

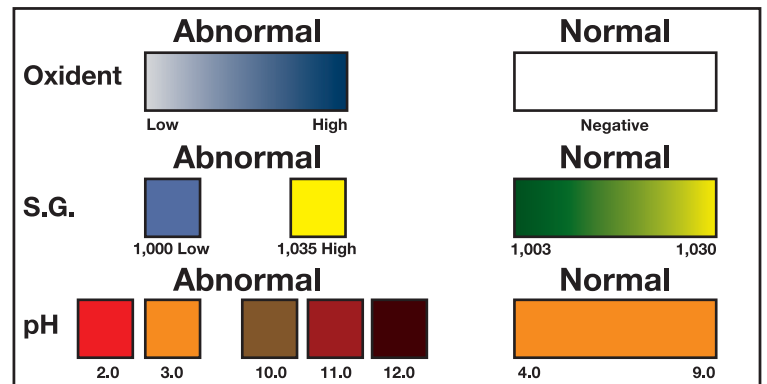

SAMPLE ONLY - Color chart NOT exact.